

FIG. 1

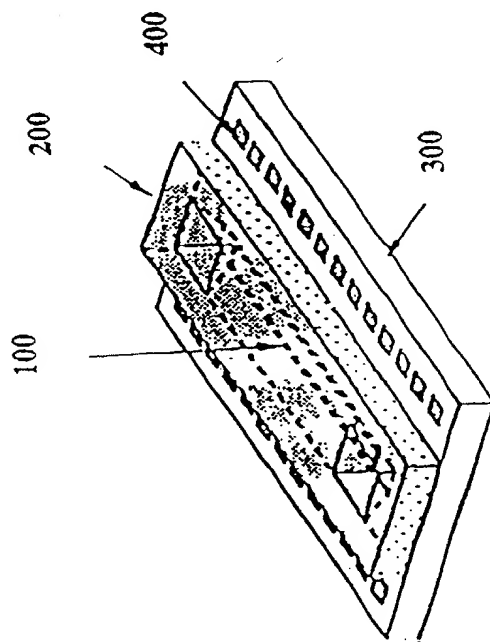


FIG. 2

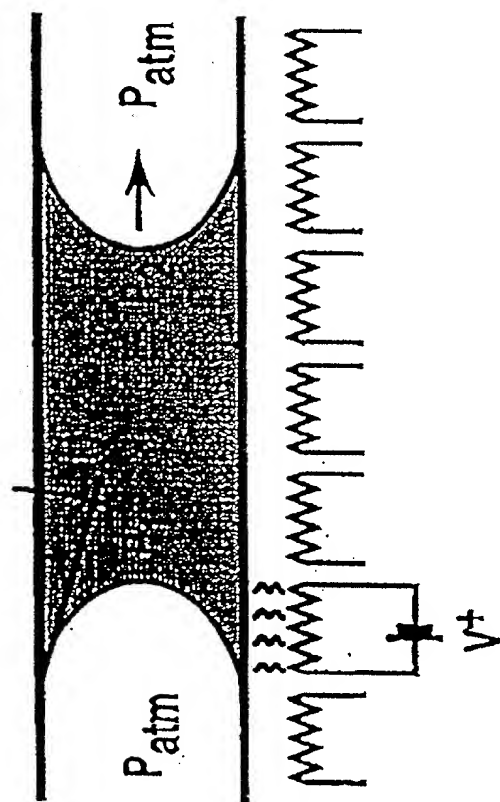


FIG. 3

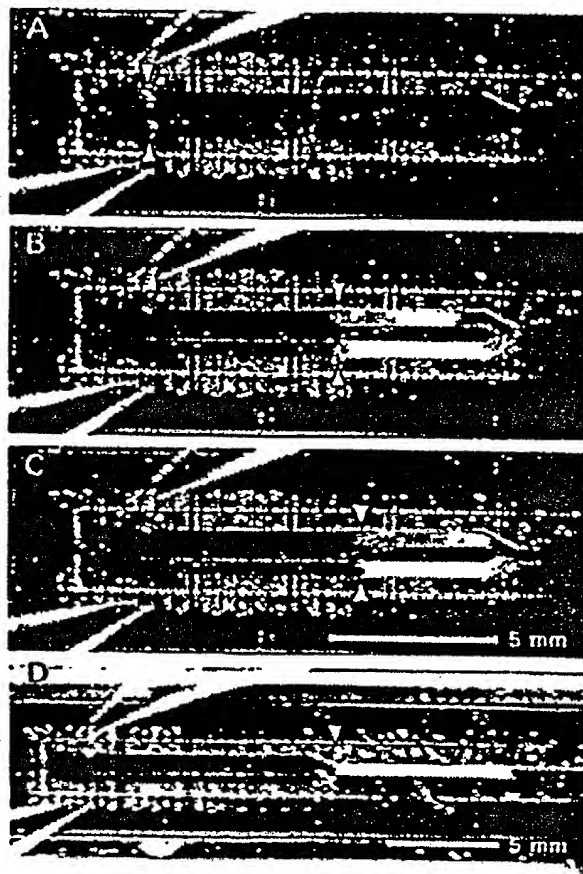


FIG. 4

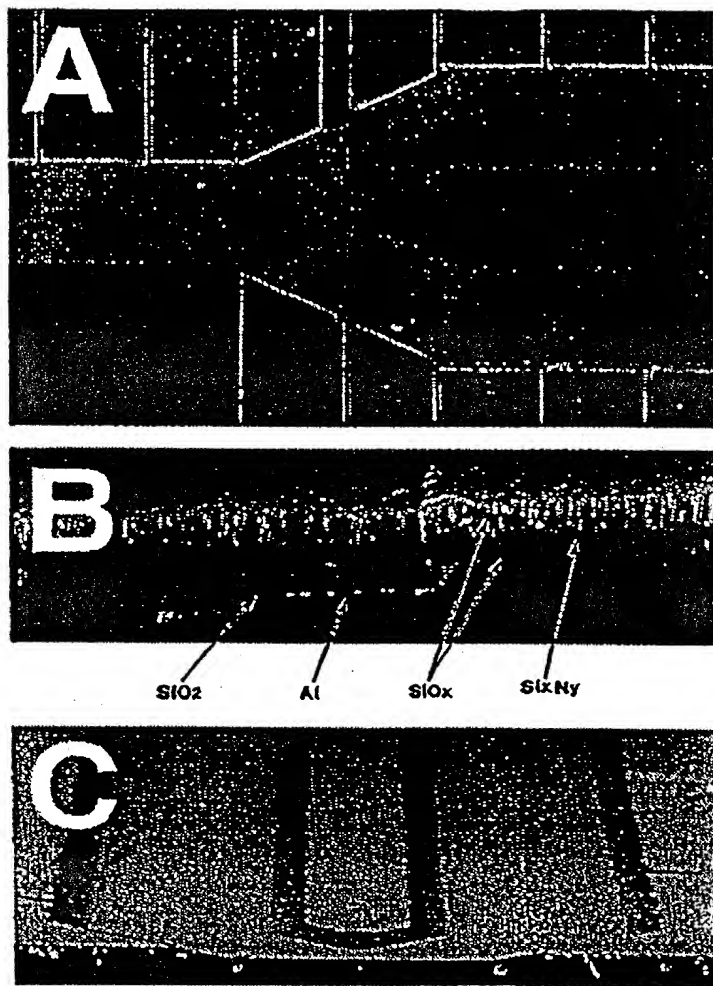


FIG. 5

08790" E64TS/60

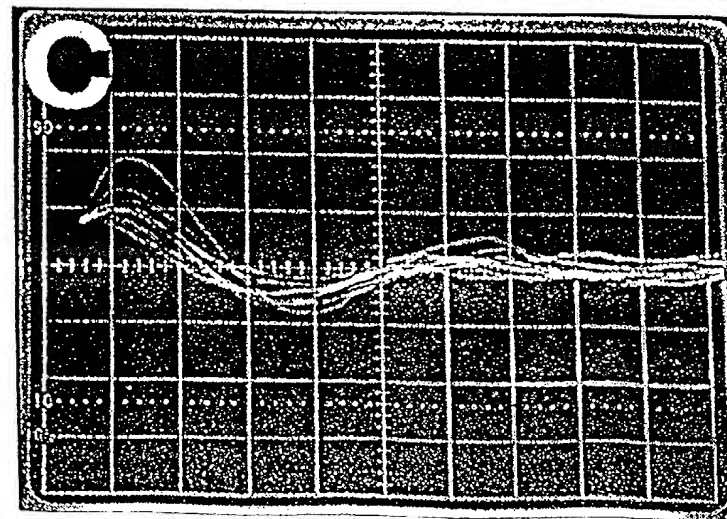
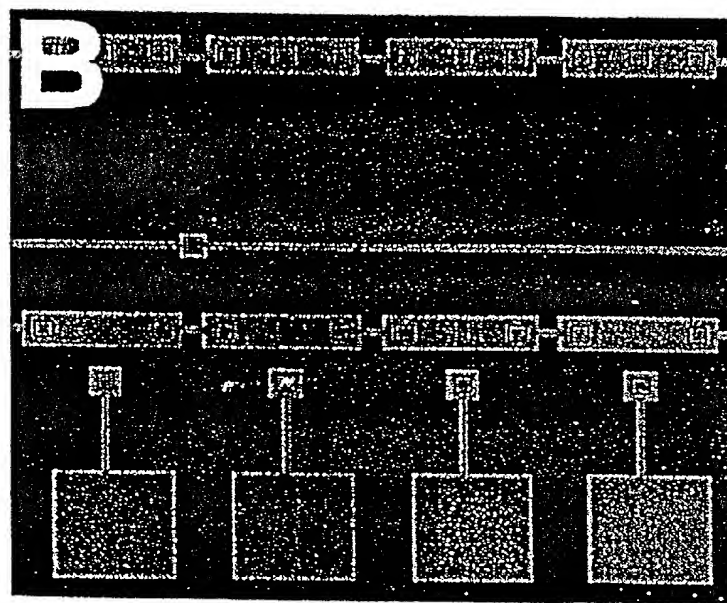
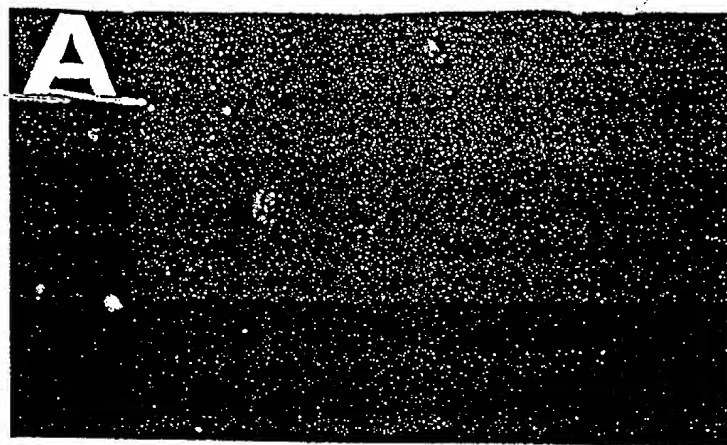


FIG. 6

# PCR Results with Standard Reagent Amounts

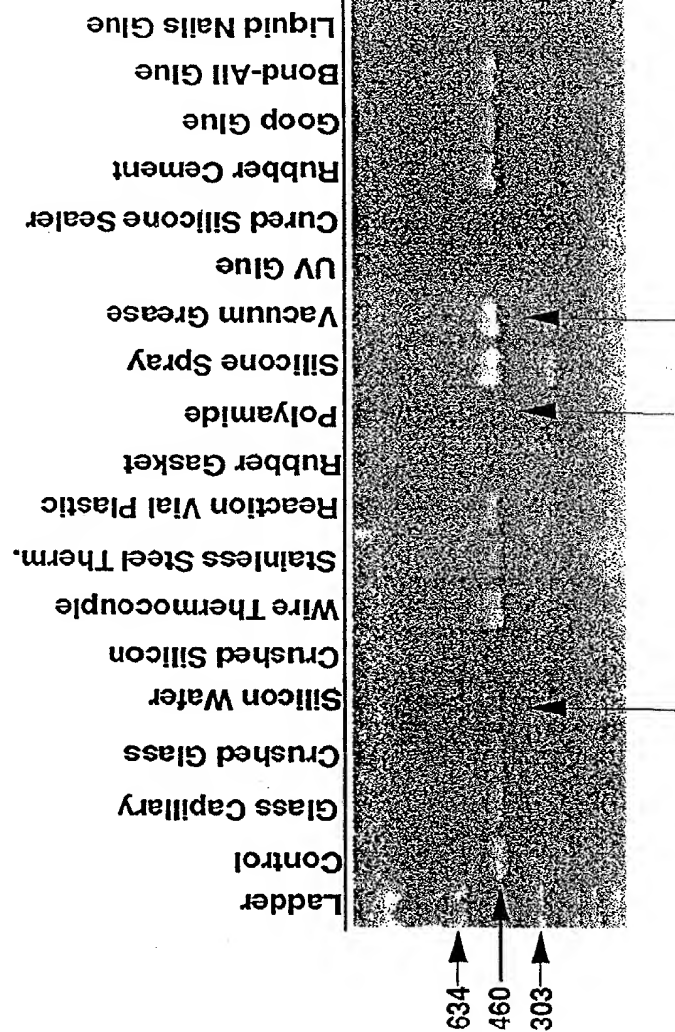


FIG. 7